




AnMar Research Laboratories B.V.

VPBEO-ARL New Product of 2009

The VPLEO

*Van Putten-**Leak** Evaluation Observatory*

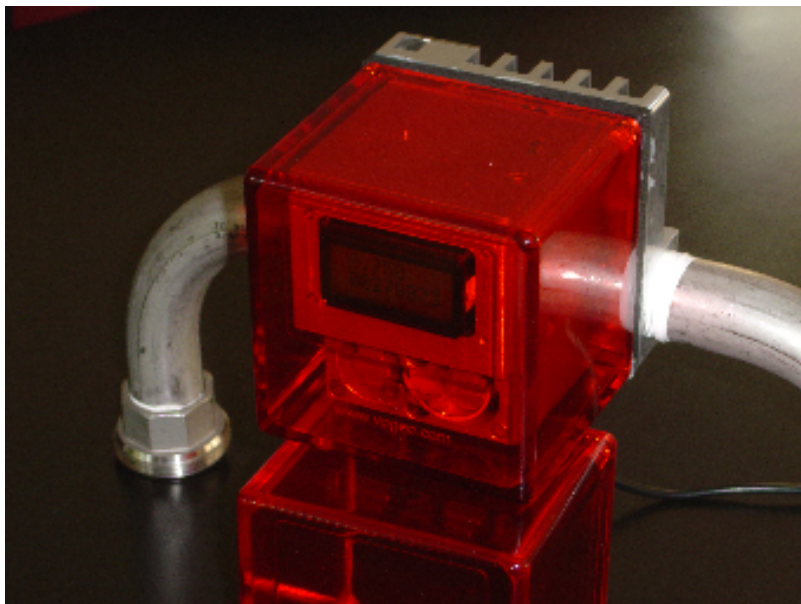

The world's most sensitive leak tester

Calibrated flow range:	0.033-25 normal ml/min
Calibration reference:	Terufusion® syringe pump STC-521
Related device certification:	CTEP/CDF A #5554-08
Uncalibrated flow range:	25-400 normal ml/min
Pressure range:	0.5-8 bar
Temperature range:	10-30 °C
Temperature compensation:	0.1 % /K (typical)
Pressure compensation:	< 0.05% /bar
Uncertainty:	1% typical
Sample frequency:	0.25 Hz
Output:	2 line display, flow rate and total normal volume
Data-transmission:	wireless (password encrypted)
Data-logging software:	VPGEO Dashboard (under Windows XP, free)